

Filip Pastorek - Miroslav Omasta – Lenka Bukovinova – Pavel Dolezal – Branislav Hadzima *

BIODEGRADATION PROPERTIES OF AZ31 MAGNESIUM ALLOY COATED BY DICALCIUM PHOSPHATE DIHYDRATE

Biodegradation properties of magnesium and its alloys that can be used for implants are not satisfactory and cause serious problems. These problems can be solved by biodegradable surface coatings. Evaluation of biodegradation process of Mg-3Al-1Zn alloy surfaces after grinding and grinding followed by potential controlled electrodeposition of dicalcium phosphate dihydrate (DCPD) was investigated by electrochemical impedance spectroscopy measurements in this study. The potentiostatic electrodeposition treatment process was performed in water solution of $\text{Ca}(\text{NO}_3)_2 \cdot 4\text{H}_2\text{O}$, $\text{NH}_4\text{H}_2\text{PO}_4$ and H_2O_2 . The corrosion process on treated and nontreated samples after various exposure times was evaluated in 0.9% NaCl solution simulating body fluid environment at 37 °C.

Keywords: Magnesium alloy, electrodeposition, calcium phosphate, electrochemical impedance spectroscopy.

1. Introduction

Magnesium is an exceptionally lightweight metal. With a density of 1.74 g/cm³, magnesium is 1.6 and 4.5 times less dense than aluminum and steel, respectively [1 - 3]. The fracture toughness of magnesium is greater than ceramic biomaterials such as hydroxyapatite, while the elastic modulus and compressive yield strength of magnesium are closer to those of natural bone than is the case for other commonly used metallic implants made of stainless steel or titanium [4 - 10]. Moreover, magnesium is essential to human metabolism and is naturally found in bone tissue. It is the fourth most abundant cation in the human body, with an estimated 1 mol of magnesium stored in the body of a normal 70 kg adult, with approximately half of the total physiological magnesium stored in bone tissue [11].

The unfortunate complication is that pure magnesium and its alloys can corrode too quickly in the physiological pH (7.4 - 7.6) and high chloride environment of the physiological system, losing mechanical integrity before the tissue has sufficiently healed and producing hydrogen gas in the corrosion process at a rate that is too fast to be dealt with by the host tissue [12]. It is likely that in spite of some early successes with magnesium-based implants [13], the metal was abandoned due to the production of gas during the in vivo corrosion process when stainless steels became available. Several possibilities exist to tailor the corrosion rate of magnesium by using alloying elements and protective coatings, processes that, of course, must lead to a non-toxic, biologically compatible material [4, 12 and 14].

Calcium phosphates have been researched extensively for biomedical applications due to their high biocompatibility and bioactivity [15]. Unfortunately, these ceramic biomaterials do not have the mechanical strength to enable them to succeed in load bearing applications. However, implant materials such as stainless steels and titanium alloys are coated with calcium phosphates [16 - 18].

Compared to conventional preparation methods, such as hot spraying or laser cladding, the structure of Ca-P coatings formed in solution is closer to that of the bone minerals [19]. Moreover, the electrodeposition technique could cost-effectively adjust the morphologies and compositions of Ca-P coatings [20].

The aim of this study is to create calcium phosphate coating on the surface of AZ31 magnesium alloy by potential-controlled electrodeposition and to evaluate the corrosion protection influence of this coating during exposure in electrolyte simulating a human body environment.

2. Experimental material and methods

Magnesium alloy AZ31 was chosen as the experimental material. It was continually cast at Brandenburgische Universität in Cottbus, Germany, heat-treated by annealing (420 °C, 6 hours) at TU Clausthal, Germany and its chemical composition was analyzed at the Magnesium innovation centre MagIC GKSS

* ^{1,2}Filip Pastorek, ¹Miroslav Omasta, ²Lenka Bukovinova, ³Pavel Dolezal, ^{1,2}Branislav Hadzima

¹Department of Materials Engineering, Faculty of Mechanical Engineering, University of Zilina, Slovakia

²Research centre of the University of Zilina, Slovakia

³Institute of Material Science and Engineering, Faculty of Mechanical Engineering, Brno University of Technology, Czech Republic

E-mail: filip.pastorek@fstroj.uniza.sk

Chemical composition of AZ31 alloy

Table 1

Component	Al	Zn	Mn	Si	Cu	Ni	Fe	Mg
wt. %	2.96	0.828	0.433	0.004	0.004	<0.001	0.002	bal.

Geesthacht, Germany. The chemical composition is listed in Table 1.

The microstructure of AZ31 alloy (Fig. 1) was observed by the CARL ZEISS AXIO Imager.A1m light metallographic microscope using AxionVision Rel 4.5 software and AxioCam MRc5 camera in the laboratories of the Department of Materials Engineering, University of Zilina. The microstructure of AZ31 alloy is created by polyedric grains of supersaturated solid solution of aluminum, zinc and other alloying elements in magnesium (solid solution δ). The average grain size is 220 μm .

AZ31 magnesium alloy samples with surface area of 2 cm^2 were ground with 500 and 1000 grit SiC paper to ensure the same surface roughness, then rinsed with demineralized water and ethanol, and dried using a stream of hot air. After described pre-treating the dicalcium phosphate dihydrate (DCPD) was deposited on the samples' surfaces. Treatment electrolyte solution was prepared with 0.1M $\text{Ca}(\text{NO}_3)_2 \cdot 4\text{H}_2\text{O}$ + 0.06M $\text{NH}_4\text{H}_2\text{PO}_4$ + 10 ml.l⁻¹ H_2O_2 . A classical three-electrode system consisting of counter electrode (platinum electrode), reference electrode (saturated calomel electrode) and working electrode (sample) was used for electrodeposition process. Electrodeposition was performed with constant potential -1.8 V vs reference electrode potential for 1 hour at room temperature 22 ± 2 °C on a laboratory apparatus VSP (producer BioLogic SAS France).

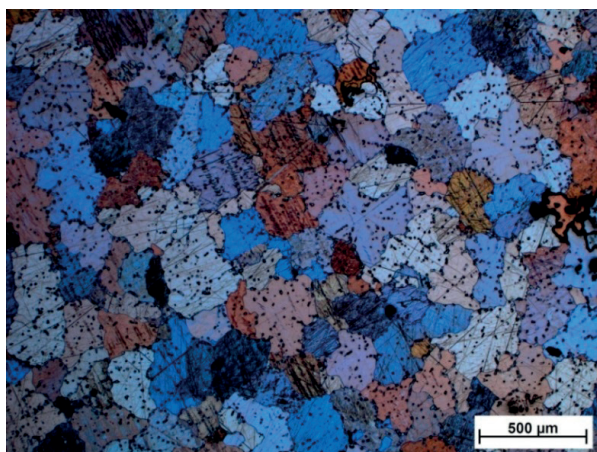


Fig. 1 Microstructure of AZ31 alloy, light microscopy, etch. picric acid + ac. acid + ethanol + water [21]

3. Results and discussion

The surface morphology of the treated samples (Fig. 2) was assessed by a stereomicroscope Nikon AZ100 with


a digital camera using NIS Elements software. As can be seen, the continuous layer of DCPD covering the entire surface is composed of irregularly branched units that overlap each other.




Fig. 2 Morphology of created calcium phosphate, light microscopy

Electrochemical impedance spectroscopy (EIS) was used for the corrosion resistance evaluation of surface layers after exposure times from 5 minutes to 168 hours in 0.9% NaCl solution at 37 ± 1 °C, which represents human body environment conditions. Corrosion electrochemical characteristics were measured and evaluated by a potentiostat/galvanostat/frequency response analyzer VSP from BioLogic SAS France. EIS measurements were performed at open circuit potential with AC voltage amplitude of 15 mV in frequency range from 100 kHz to 10 mHz.


Results from EIS measurements in the form of impedance and phase Bode plots are shown in Fig. 3 and Fig. 4 for AZ31 samples with ground surface and surface coated by DCPD, respectively. Bode plots were analyzed by software EC-Lab V10.12 using equivalent circuits. Fig. 5 expresses the equivalent circuit used for the analysis of Bode plots with one minimum in *phase shift vs log f* interpretation and Fig. 6 the equivalent circuit used for the analysis of Bode plots with two minimums in *phase shift vs log f* interpretation [3]. These equivalent circuits use various elements expressing the character of evaluated surface. In our case, R_Ω is resistance of the solution, R_{p1} and R_{p2} are polarization resistances of various mechanisms in corrosion model (e.g. charge transfer, film resistance,...), R_p is mixed polarization resistance or sum of partial polarization resistances ($R_{p1} + R_{p2}$) and CPE_1 and CPE_2 are constant phase elements of mechanisms corresponding with R_{p1} and R_{p2} , respectively. CPE_1 in second equivalent circuit is constant phase element of the layer of corrosion products.

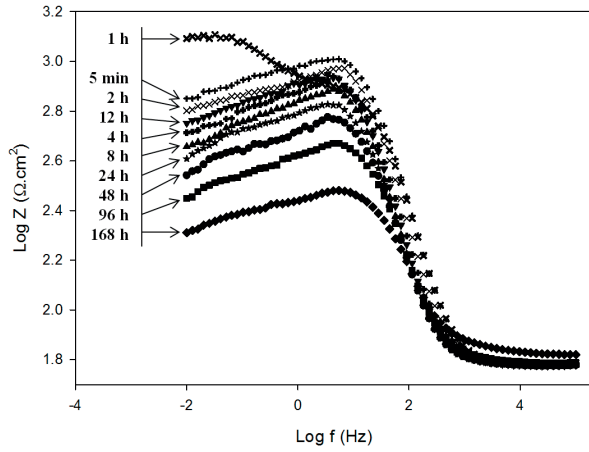

a)

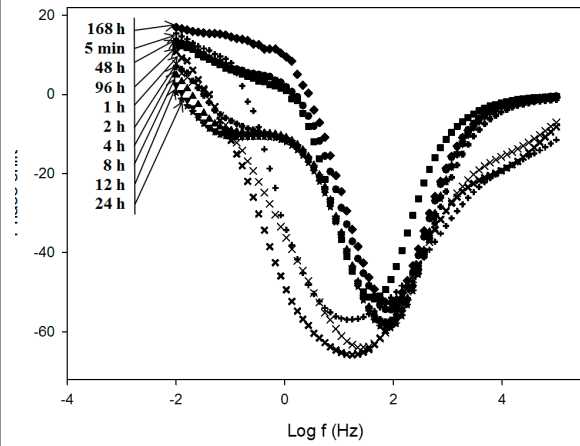


b)

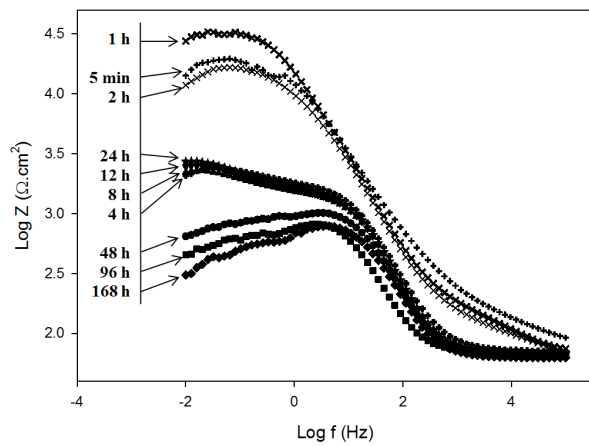

b)

Fig. 3 Impedance Bode plots of AZ31 samples: a) Ground surface, b) Surface with DCPD layer

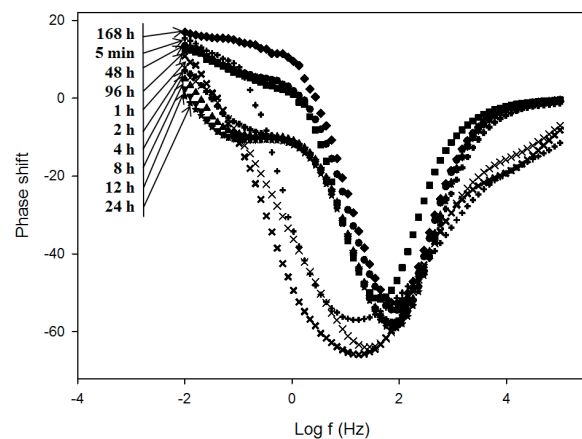

a)

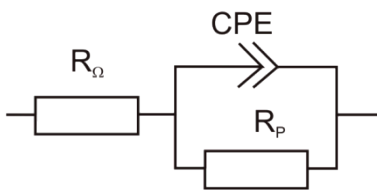


Fig. 5 Equivalent circuit used for the analysis of Bode plots with one minimum in phase shift vs log f interpretation

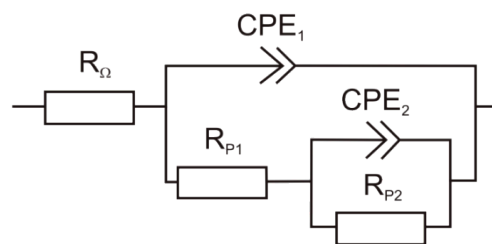


Fig. 6 Equivalent circuit used for the analysis of Bode plots with two minima in phase shift vs log f interpretation

Based on Bode plots analysis the values of polarization resistance R_p were obtained. This electrochemical characteristic represents the corrosion resistance of the surface layer (or layers). The values of polarization resistances and other electrochemical characteristics gained after various exposure times on AZ31 magnesium alloy samples without and with DCPD coating are listed in Table 2.

Polarization resistance values of the ground AZ31 samples and ground AZ31 samples with DCPD surface layer after various exposure times (0.9% NaCl)

Table 2

	5min	1 h	2 h	4 h	8 h	12 h	24 h	48 h	96 h	168 h
$R_p (\Omega \cdot \text{cm}^2)$ ground	1059	1239	985	825	729	836	625	539	410	241
$R_p (\Omega \cdot \text{cm}^2)$ ground + DCPD	19047	34972	16868	2421	2236	2664	2729	953	772	730

A formation of the surface layer of corrosion products based on magnesium oxide (MgO) and hydroxide (Mg (OH)₂) was observed in a short time after the immersion of the ground AZ31 sample in 0.9% NaCl at 37 °C. This formation resulted in the increase of polarization resistance R_p values which is terminated after 1 hour of exposure when the maximum value of R_p (1239 $\Omega \cdot \text{cm}^2$) was reached. By increase of exposure time the gradual decrease of R_p values is observed up to a minimum 241 $\Omega \cdot \text{cm}^2$ measured after 168 hours of exposure. The decrease of R_p values can be explained by the degradation of the surface layer formed of corrosion products and by the subsequent local corrosion attack realized by aggressive components of electrolyte.

AZ31 samples with DCPD surface layer showed substantial increase of polarization resistance R_p values after various exposure times in corrosive environment at 37 °C compared to ground AZ31 samples. The value of R_p (19047 $\Omega \cdot \text{cm}^2$) reached on the surface with DCPD layer after 5 minutes of exposure was 19 - fold higher compared to ground samples at the same exposure. Maximal polarization resistance value R_p (34972 $\Omega \cdot \text{cm}^2$) reached after 1 hour of exposure represented more than 29 times higher value compared to the maximal value of R_p reached on ground samples. Corrosion process of the samples with DCPD surface layer is different from the corrosion process of ground samples. At the moment of the samples immersion a reaction of DCPD with the corrosive medium (0.9% NaCl, 37 °C) and the formation of corrosion products in places with insufficient DCPD coverage occurred. These two processes resulted in filling imperfections in the DCPD layer thus increasing the polarization resistance R_p . After 2 hours of exposure there was a decrease in R_p values (to 16868 $\Omega \cdot \text{cm}^2$) caused by a gradual degradation of the surface resulting in local increase of corrosion activity in the weakest DCPD locations. This gradual decrease of R_p values caused by ongoing DCPD dissolution and more intensive corrosion continued till the end of the immersion test after 168 hours when the minimal value of R_p was reached (730 $\Omega \cdot \text{cm}^2$). Despite of significant loss of DCPD corrosion protection after longer exposure times, the polarization resistance values of the surface with DCPD layer are significantly higher after all exposure times compared to ground surface.

5. Conclusions

On the basis of performed experiments, analysis of the results and their interpretations, we came to the following conclusions:

1. Thin calcium phosphate dihydrate (DCPD) coating prepared by potential-controlled electrodeposition process under specified conditions forms the continuous layer composed of irregularly branched flake-like formations of a different size covering the entire surface.
2. The polarization resistance (R_p) value of AZ31 samples with DCPD coating (19047 $\Omega \cdot \text{cm}^2$) reached after first 5 minutes of exposure in corrosive medium achieves 19-fold higher value compared to that of ground samples (1059 $\Omega \cdot \text{cm}^2$) after the same exposure time which represents a relevant improvement of surface layer corrosion protection.
3. Maximum value of R_p reached on samples with DCPD coating after 1 hour of exposure (34972 $\Omega \cdot \text{cm}^2$) is 29 times higher than the maximum R_p value of the samples with ground surface (1239 $\Omega \cdot \text{cm}^2$) recorded also after this exposure time.
4. Prepared DCPD coating provides significant corrosion protection in 0.9% NaCl solution at 37 °C for 4 hours of exposure. Consequently, there is a gradual degradation of the coating and local corrosion processes as evidenced by decrease in polarization resistance values.
5. This surface layer provides higher corrosion resistance of the AZ31 surface layer at all of the selected exposure times when there is still a 3-fold higher value of R_p measured on samples with DCPD coating compared to ground samples after maximal exposure time 168 hours.

Acknowledgements

The research is supported by European regional development fund and Slovak state budget by the project: Research centre of the University of Zilina, ITMS 26220220183 and Unique equipment for evaluation of tribological properties of machines parts surfaces, ITMS 26220220048. Authors are grateful for the support of experimental works by project VEGA No. 1/0831/13.

References

- [1] DEGARMO, P. E.: *Materials and Processes in Manufacturing*, 5th ed., New York: Collin Macmillan, 1979.
- [2] HLAVACOVA, I., PALCEK, P., CHALUPOVA, M., DRESSLEROVA, Z.: *Manufacturing Technology*, 13, 2013, 313-319.
- [3] JANECEK, M., KRAL, R., DOBRON, P., CHMELIK, F., SUPIK, V., HOLLANDER, F.: *Mater. Sci. Eng.: A* 462, 2007, 311-315.
- [4] PASTOREK, F., HADZIMA, B.: *Mater. Eng. - Mater. inz.* 20, 2013, 54-63.
- [5] SARIS, N. E. L.: *Clin. Chim. Acta* 294, 2000, 1-26.
- [6] OKUMA, T.: *Nutrition* 17, 2001, 679-680.
- [7] VORMANN, J.: *Mol. Aspects Med.* 24, 2003, 27-37.
- [8] CZAN, A., SAJGALIK, M., HOLUBJAK, J., KOURIL, K.: *Manufacturing Technology* 13, 2013, 428-431.
- [9] BRONCEK, J., DZIMKO, M., HADZIMA, B., TAKEICHI, Y.: *Acta Metallurgica Slovaca* 20, 2014, 97-104.
- [10] HALAMOVA, M., LIPTAKOVA, T., ALASKARI, A., BOLZONI, F.: *Communications - Scientific Letters of the University of Zilina*, vol. 16, 2014, 78-83.
- [11] HARTWIG, A.: *Mutat Res/Fund Mol Mech Mutagen* 475, 2001, 113-121.
- [12] WITTE, F., KAESE, V., HAFERKAMP, H., SWITZER, E., MEYER-LINDENBERG, A., WIRTH, C. J.: *Biomaterials* 26, 2005, 3557-3563.
- [13] MCBRIDE, E. D.: *J Am Med Assoc* 111, 1938, 2464-2467.
- [14] HADZIMA, B., BUKOVINA, M., DOLEZAL, P.: *Mater. Eng. - Mater. inz.* 17(4), 2010, 14-19.
- [15] BEST, S. M., PORTER, A. E., THIAN, E. S., JUANG, J.: *J. Eur. Ceram. Soc.* 28, 2008, 1319-1327.
- [16] YEN, S. K., KUA, M. C.: *Mater. Sci. Eng. C* 20, 2002, 153-160.
- [17] LIU, D.-M., YANG, Q., TROCZYNSKI, T.: *Biomaterials* 23, 2002, 691-698.
- [18] KANNAN, M. B., WALLIPA, O.: *Mater. Sci. Eng. C* 33, 2013, 675-679.
- [19] ZHANG, J. M., LIN, C. J., FENG, Z. D., TIAN, Z. W.: *J Electroanal Chem* 452, 1998, 235-40.
- [20] SONG, Y., ZHANG, S., LI, J., ZHAO, Ch., ZHANG, X.: *Acta Biomaterialia* 6, 2010, 1736-1742.
- [21] NOVY, F., JANECEK, M., SKORIK, V., MULLER, J., WAGNER, L.: *Int. J. Mater. Res.* 100, 2009, 288-291.